

1/18

FIG. 1

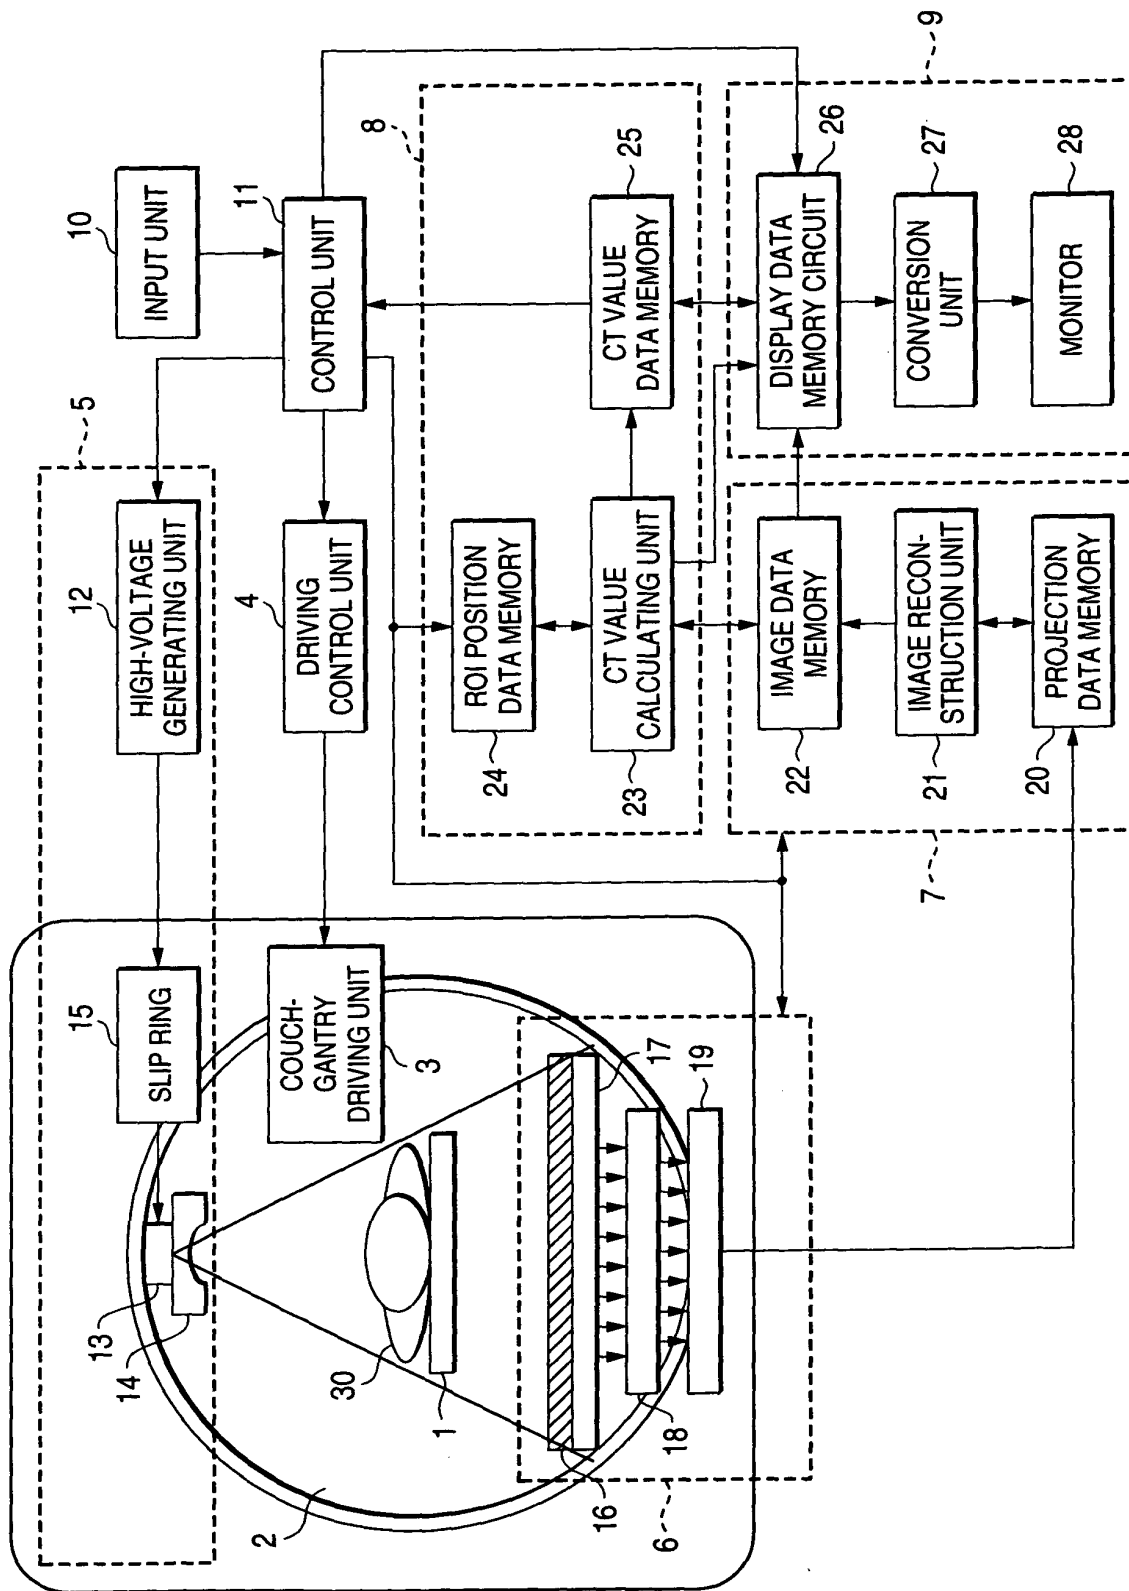


FIG. 2A



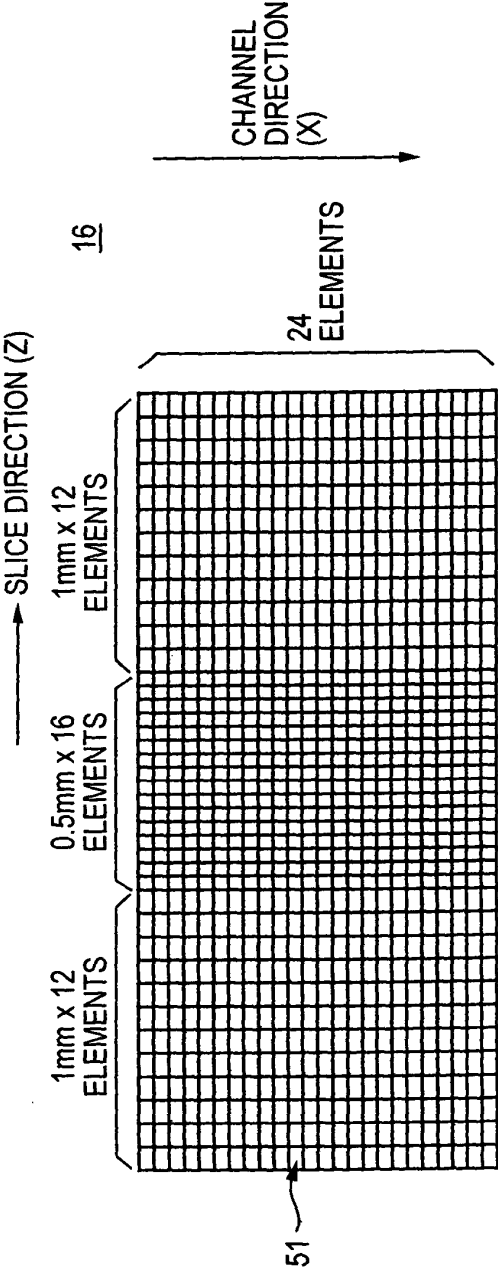


FIG. 2B

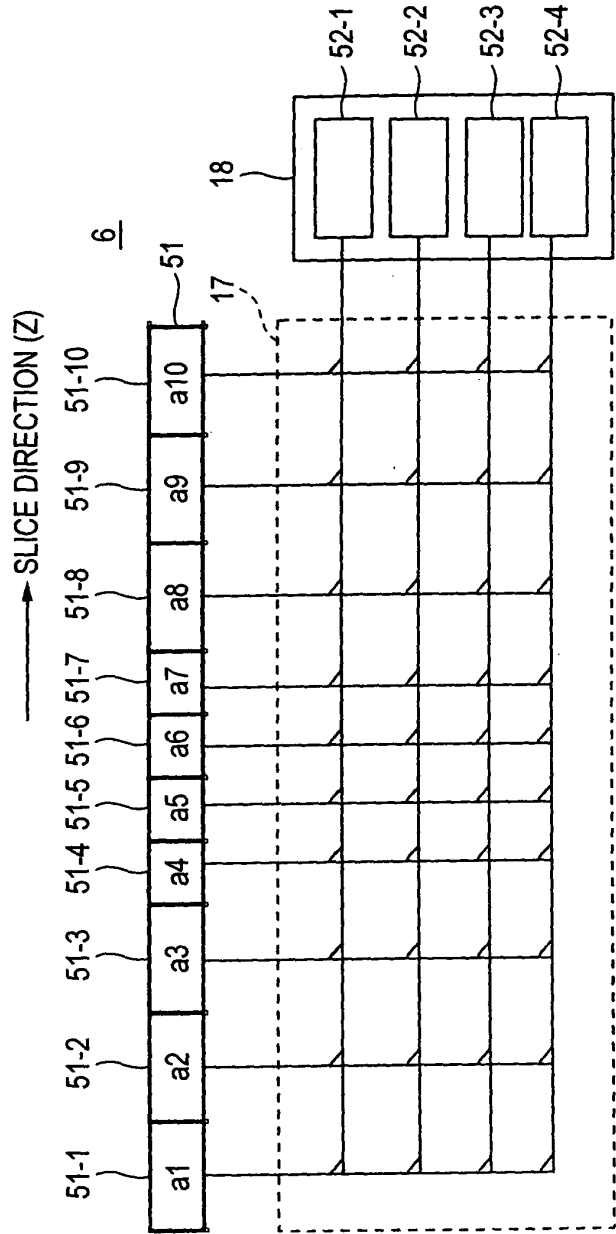

3/18

FIG. 3

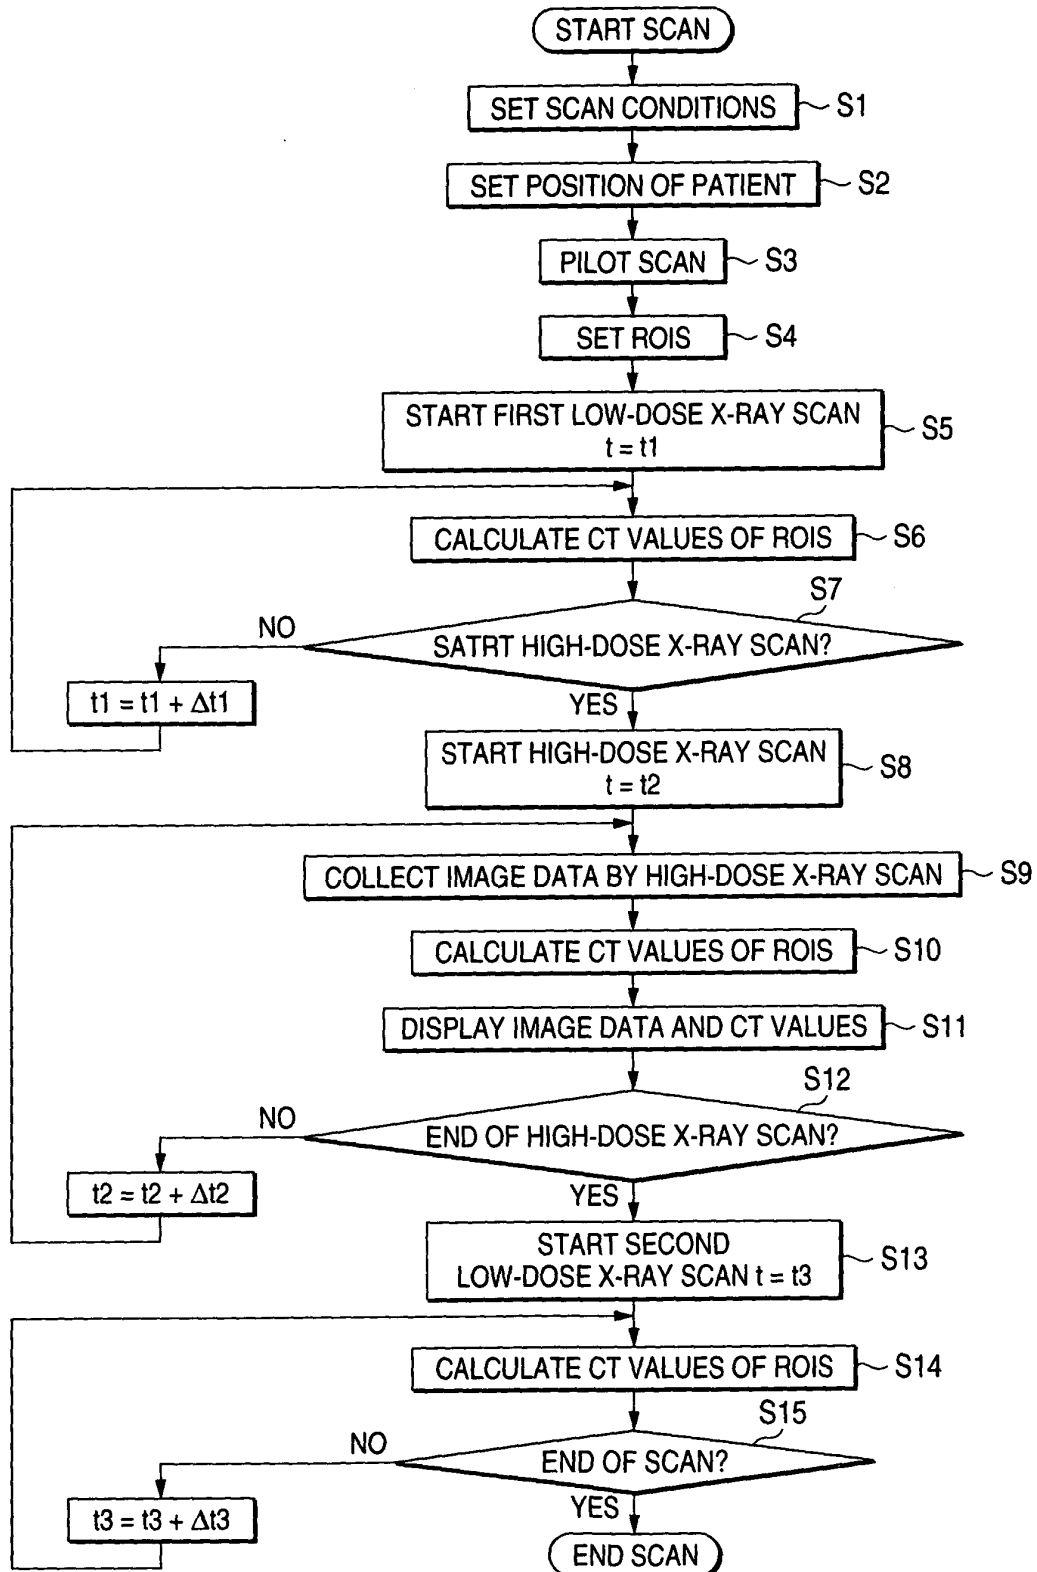


4/18

FIG. 4


	TUBE VOLTAGE	TUBE CURRENT	INTER-SCAN INTERVAL
FIRST LOW-DOSE X-RAY SCAN	120kV	50mA	2 SECONDS
HIGH-DOSE X-RAY SCAN	120kV	100mA	1 SECOND
SECOND LOW-DOSE X-RAY SCAN	120kV	70mA	2 SECONDS

FIG. 5

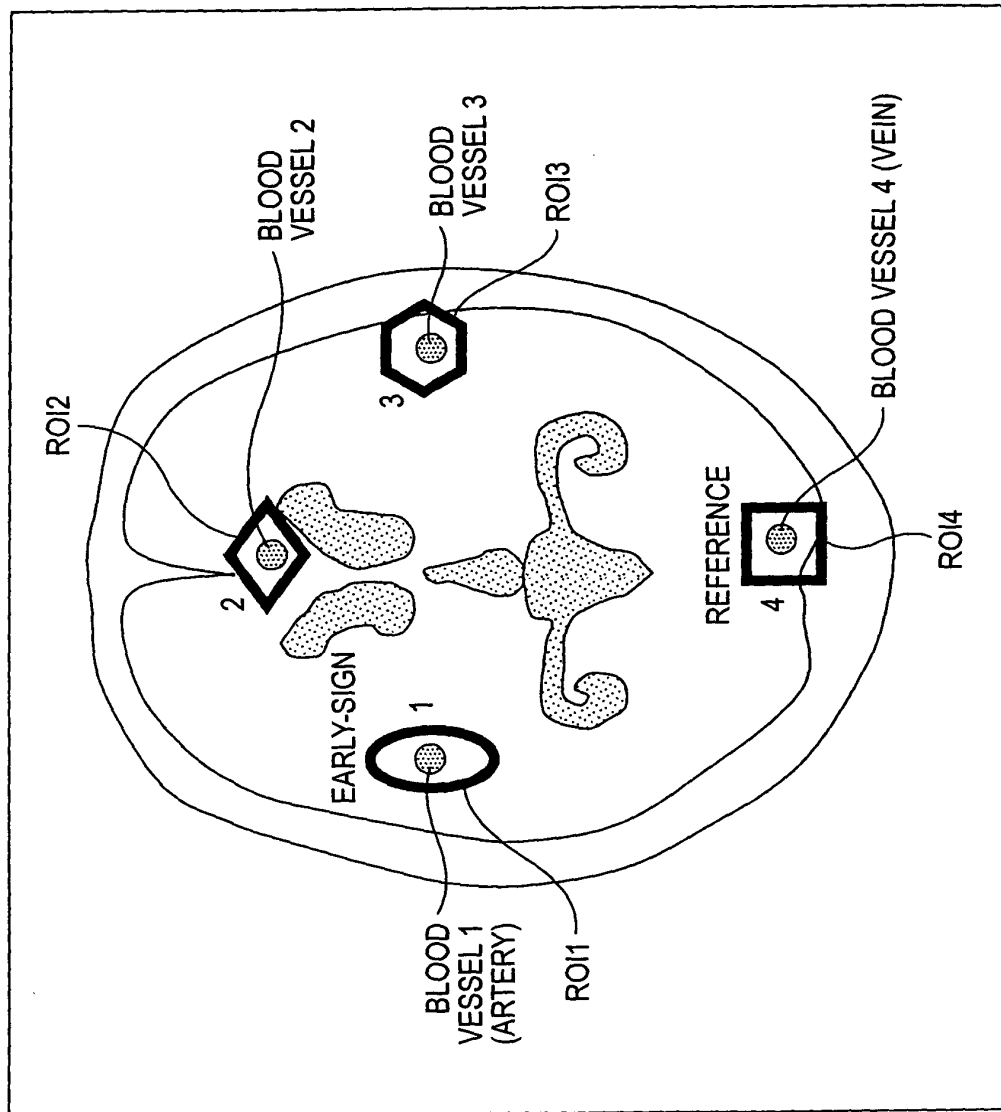


6/18

FIG. 6

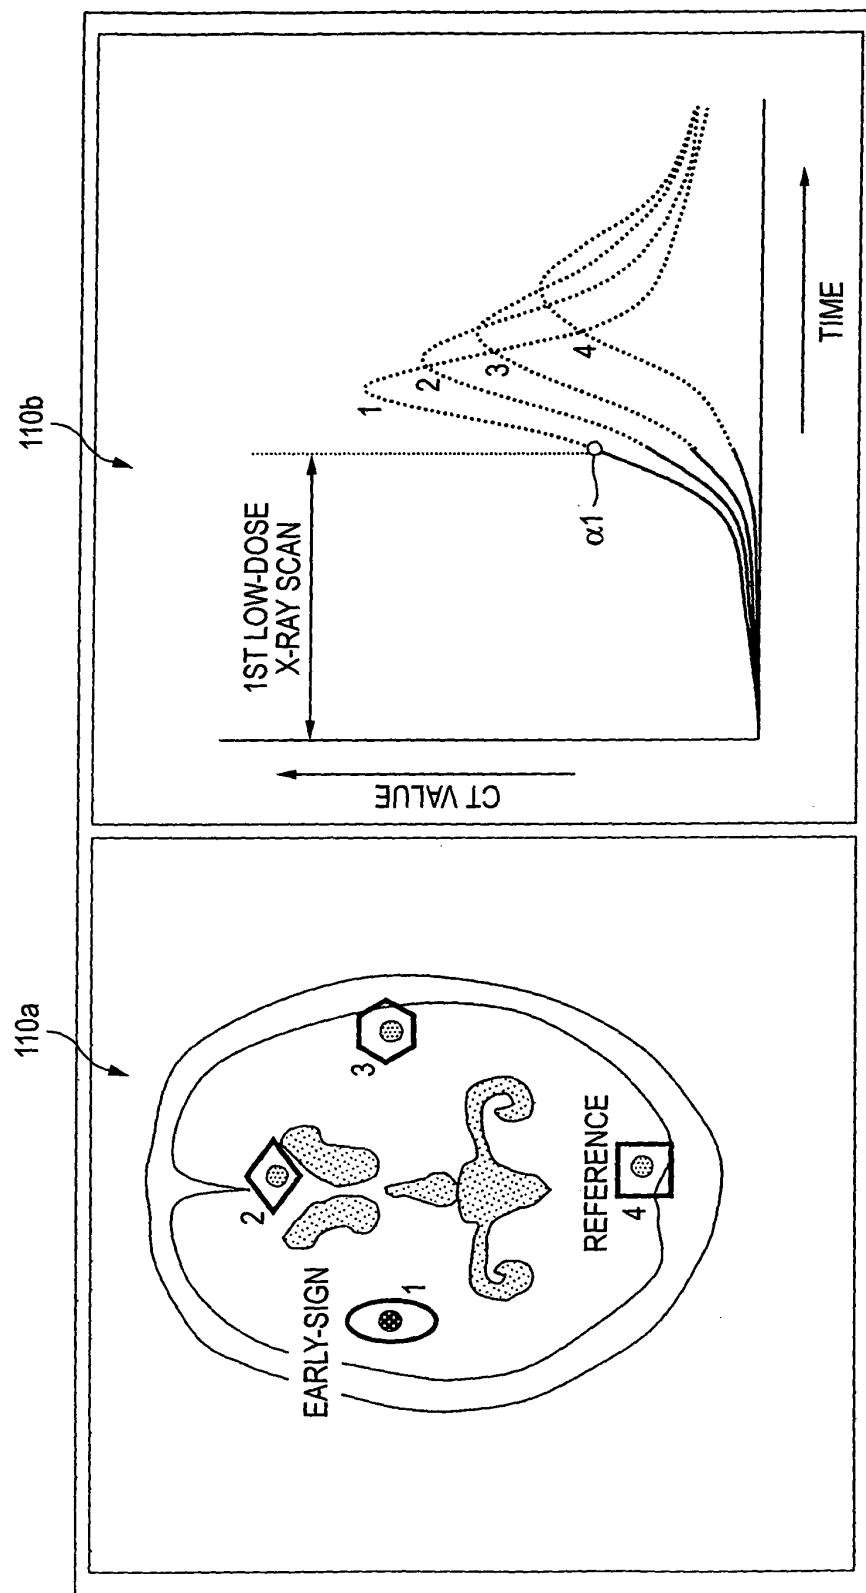


7/18

FIG. 7

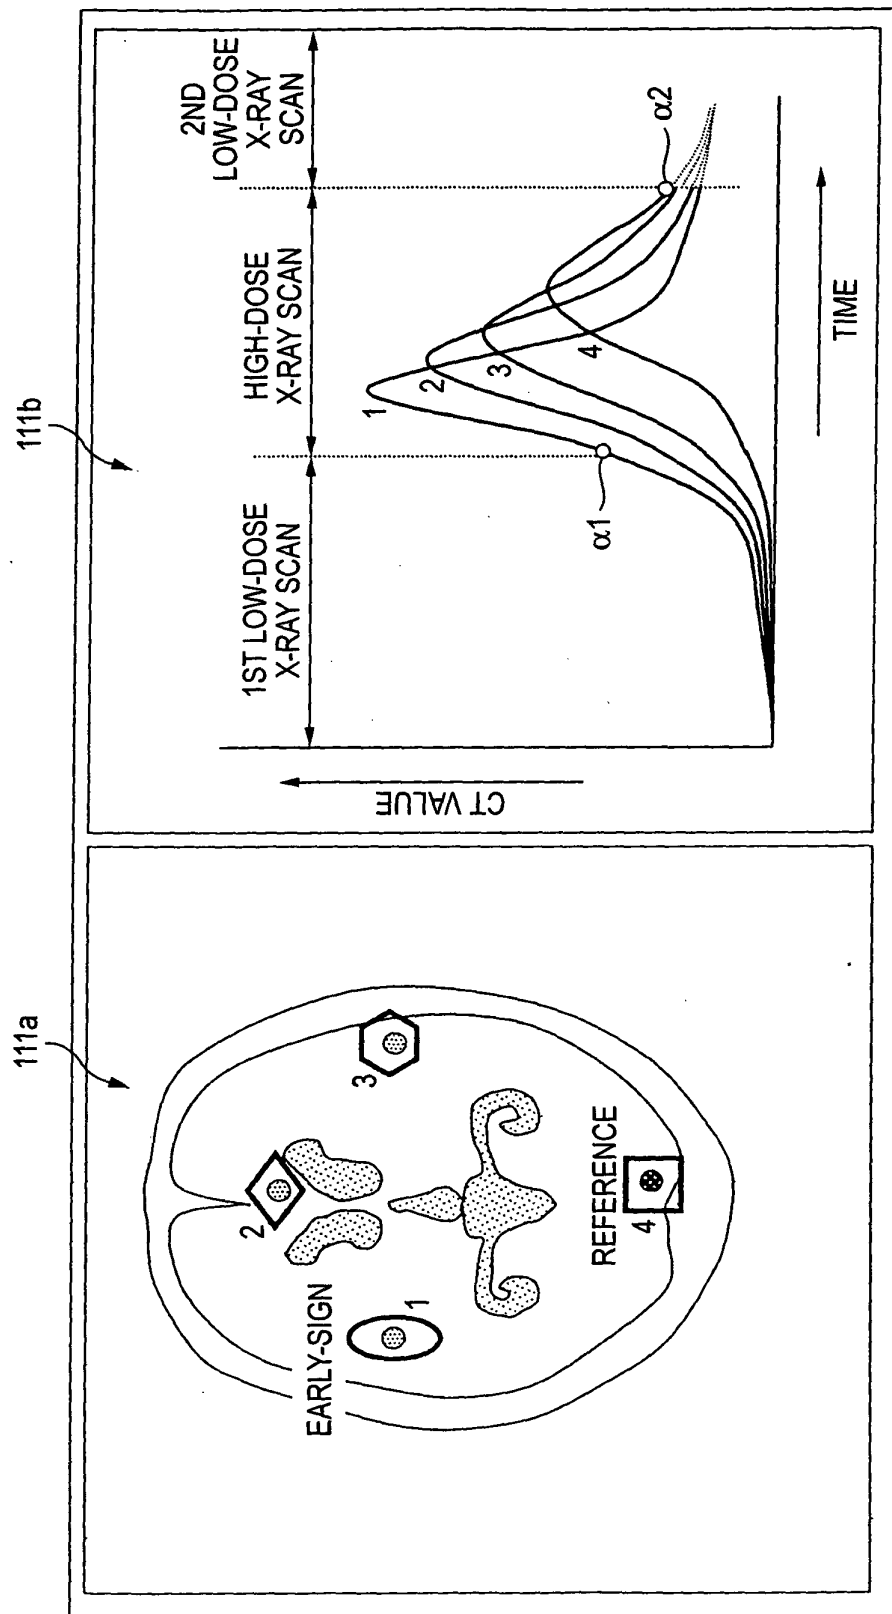


8/18

FIG. 8

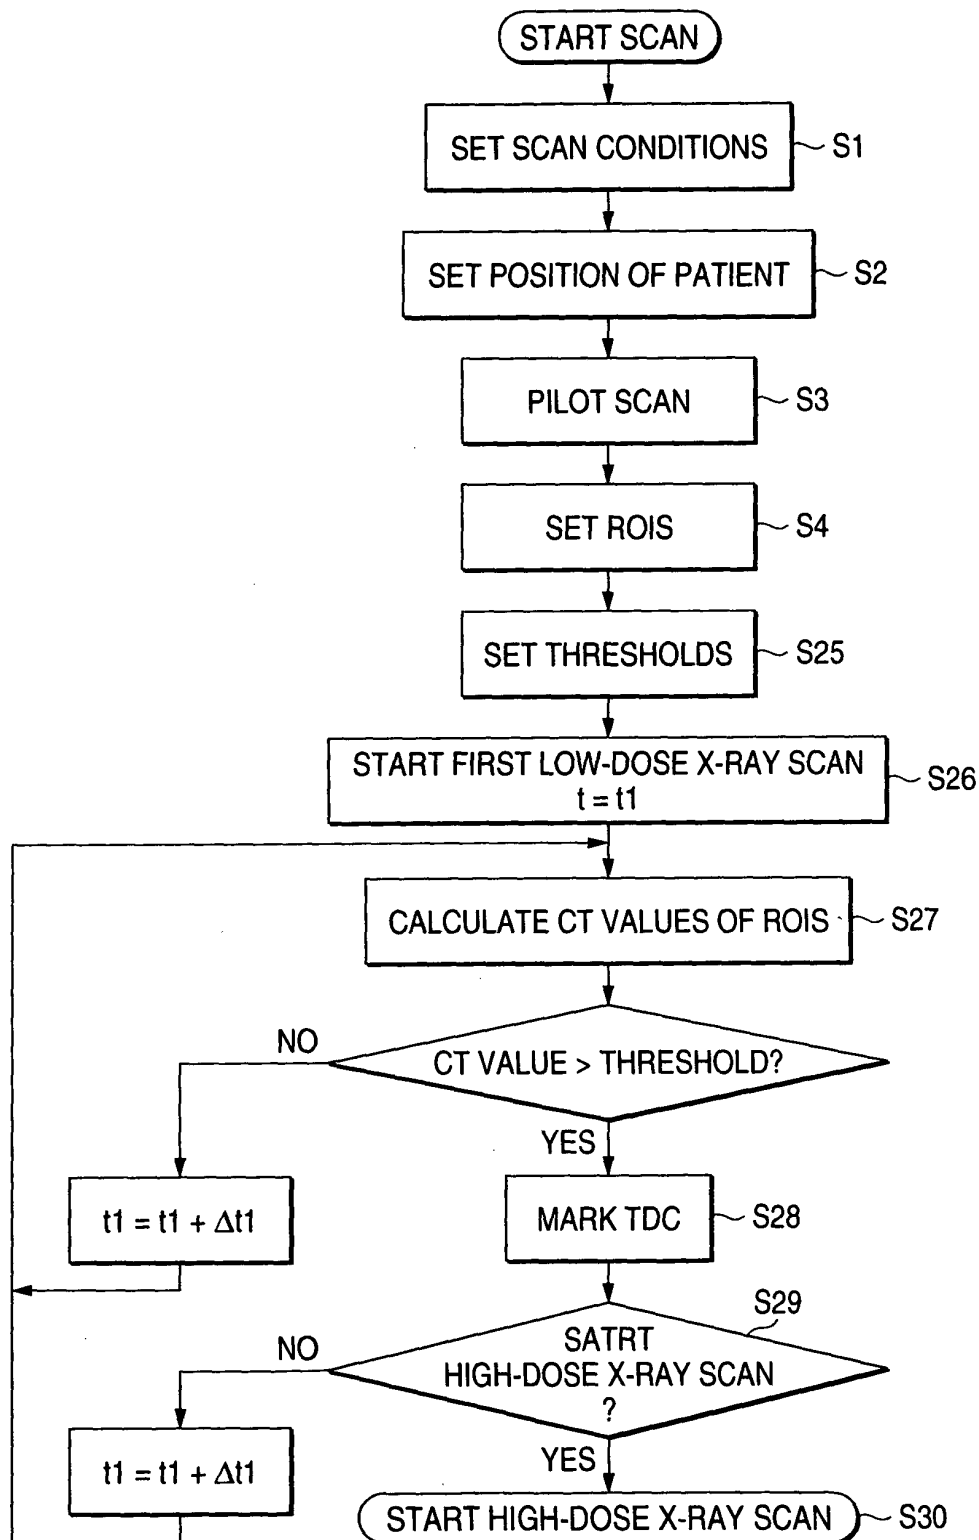


9/18

FIG. 9

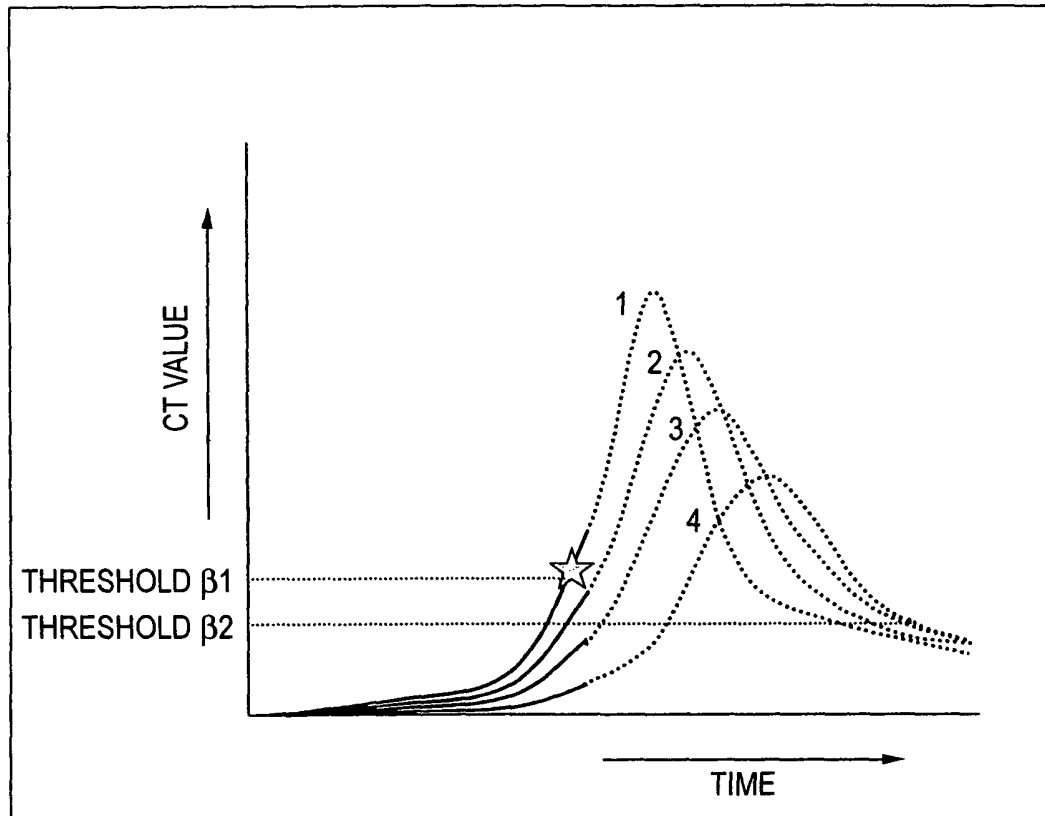


10/18

FIG. 10

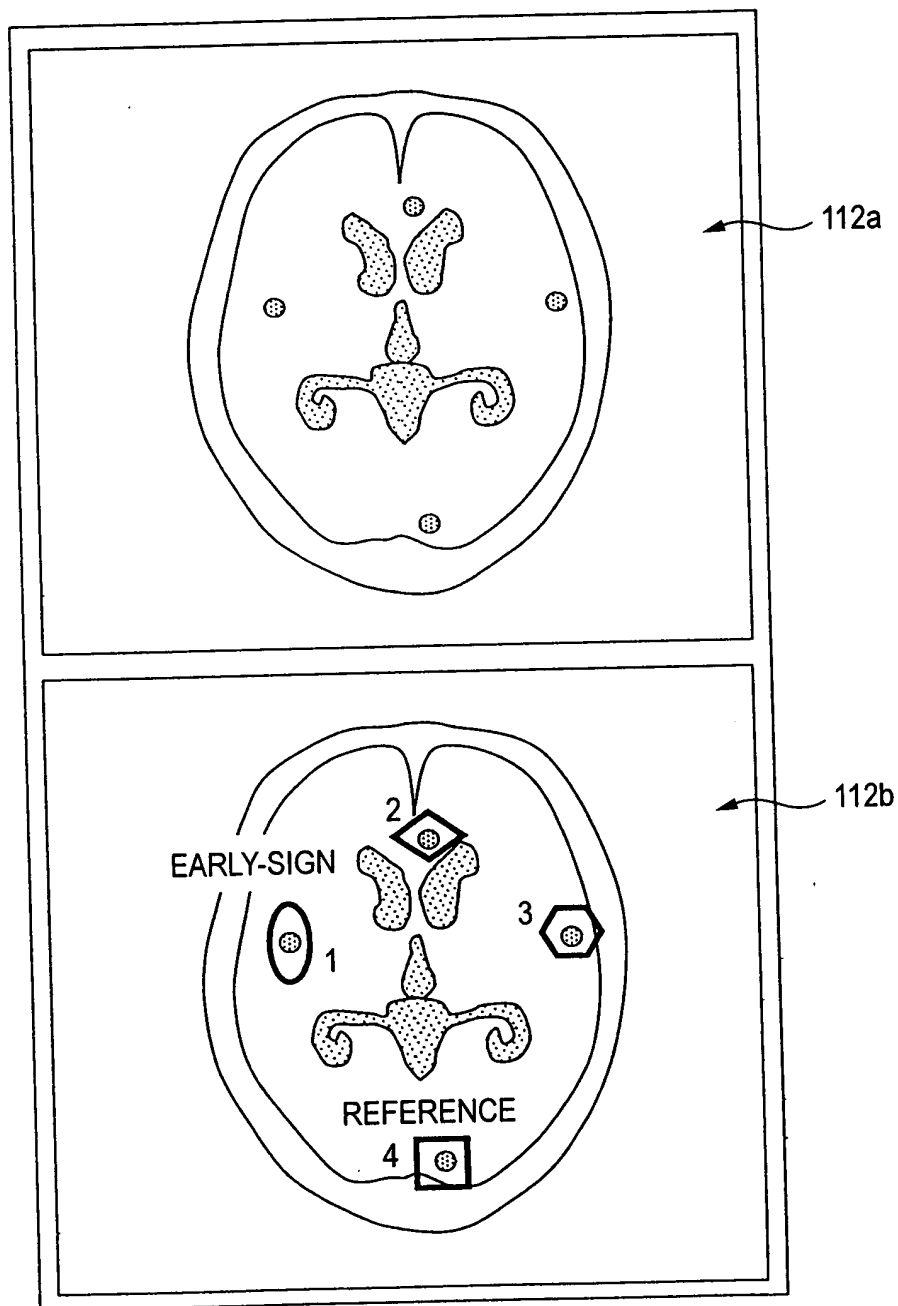


11/18

FIG. 11

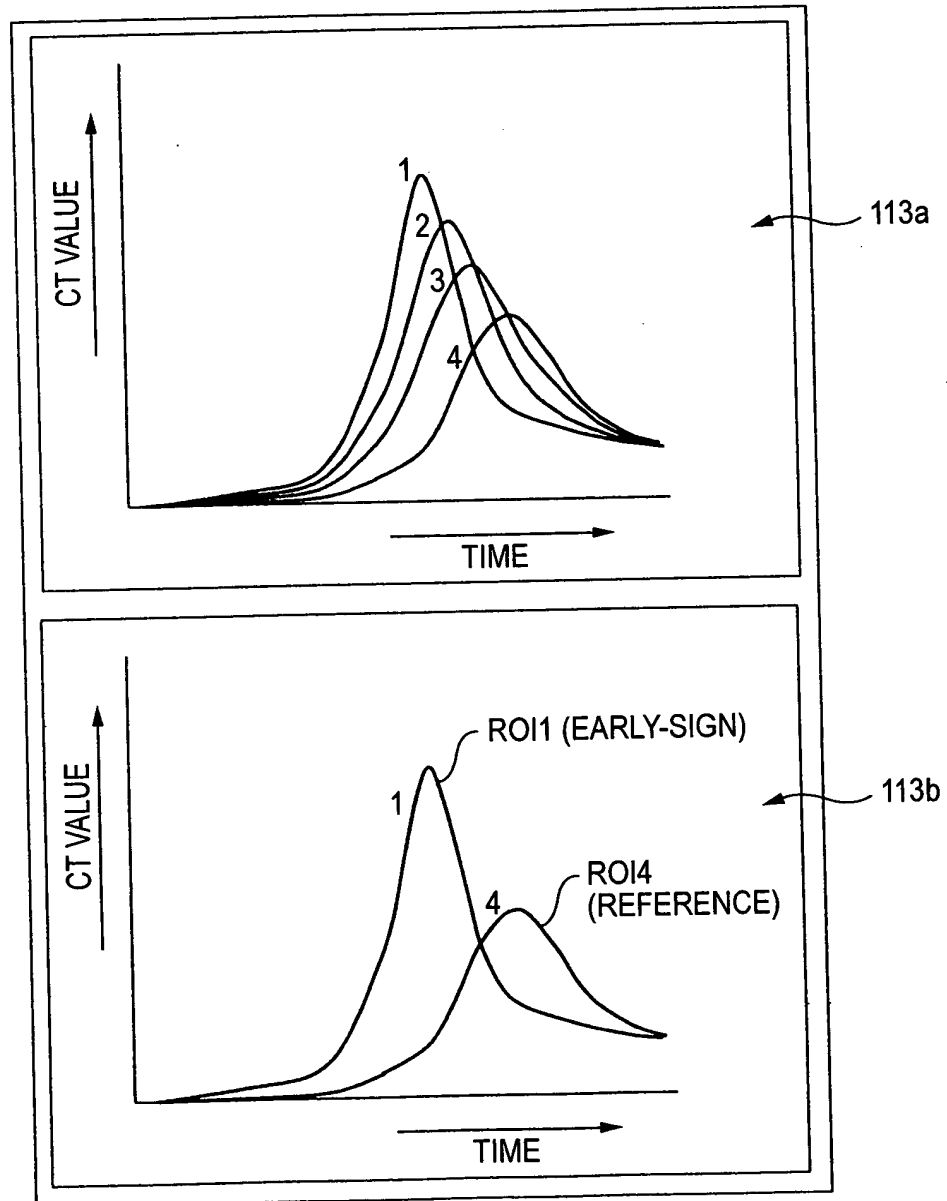

12/18

FIG. 12

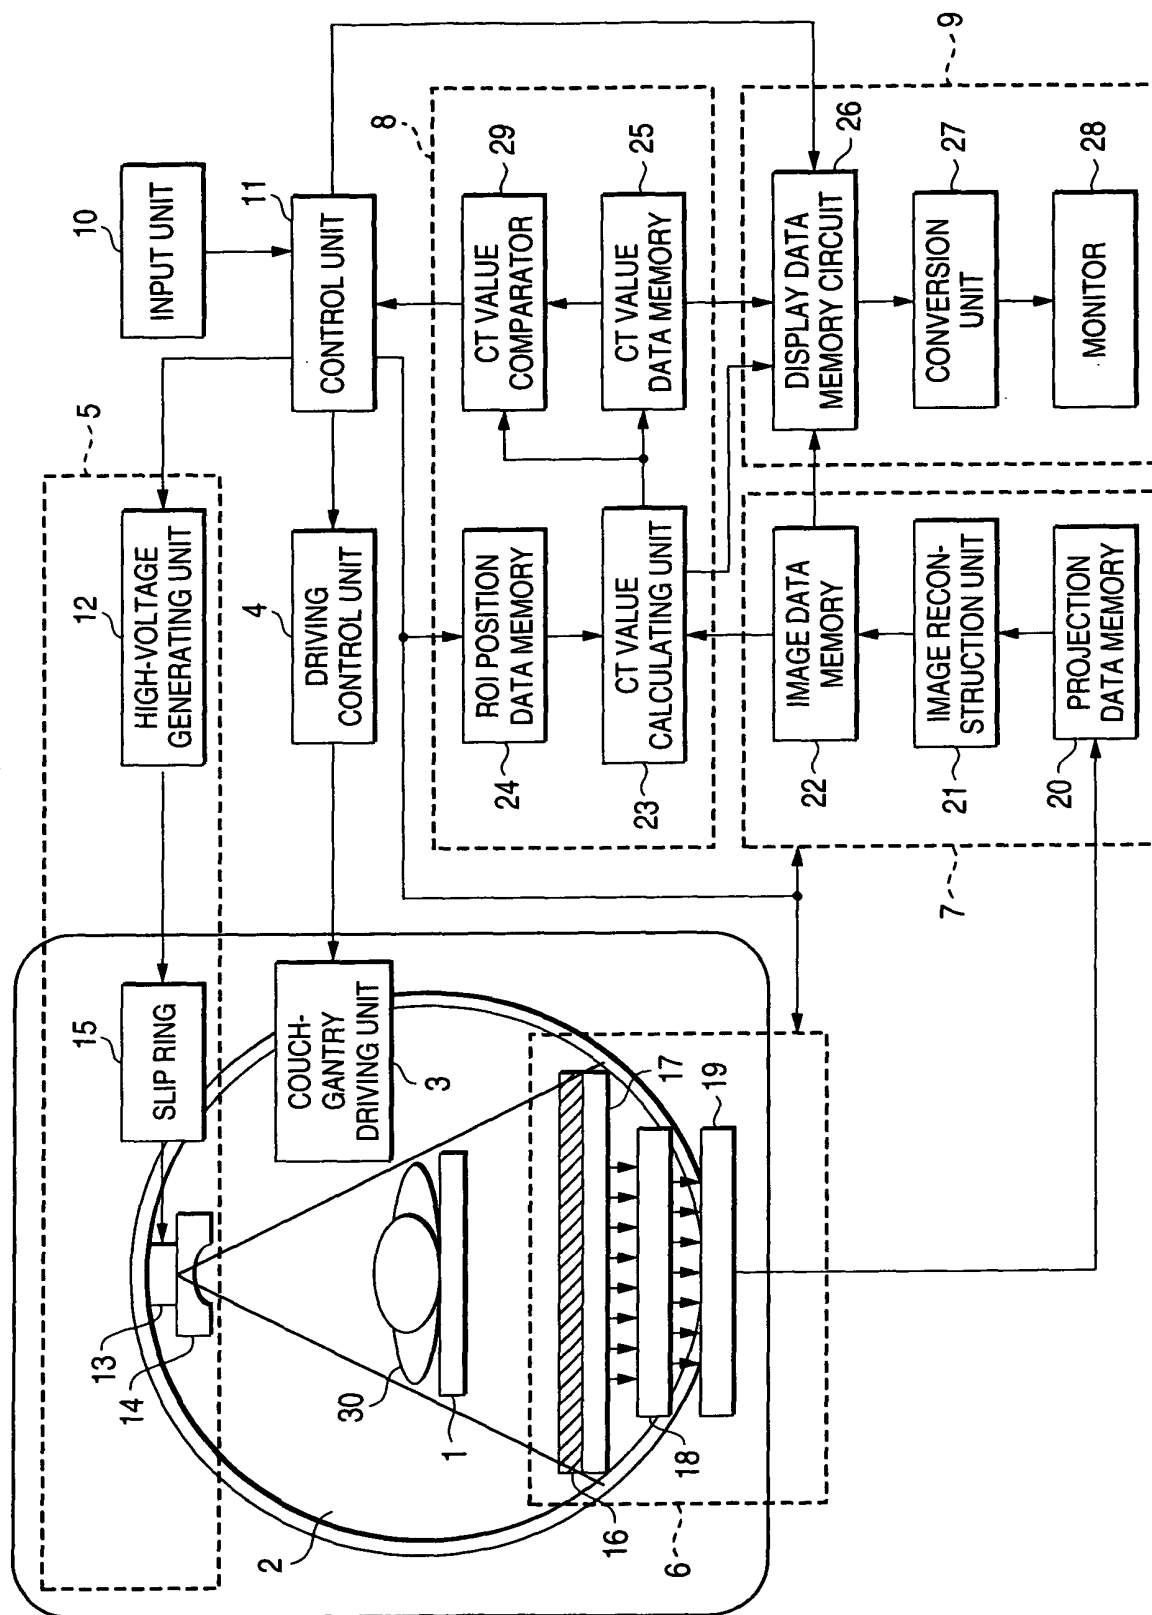

13/18

FIG. 13

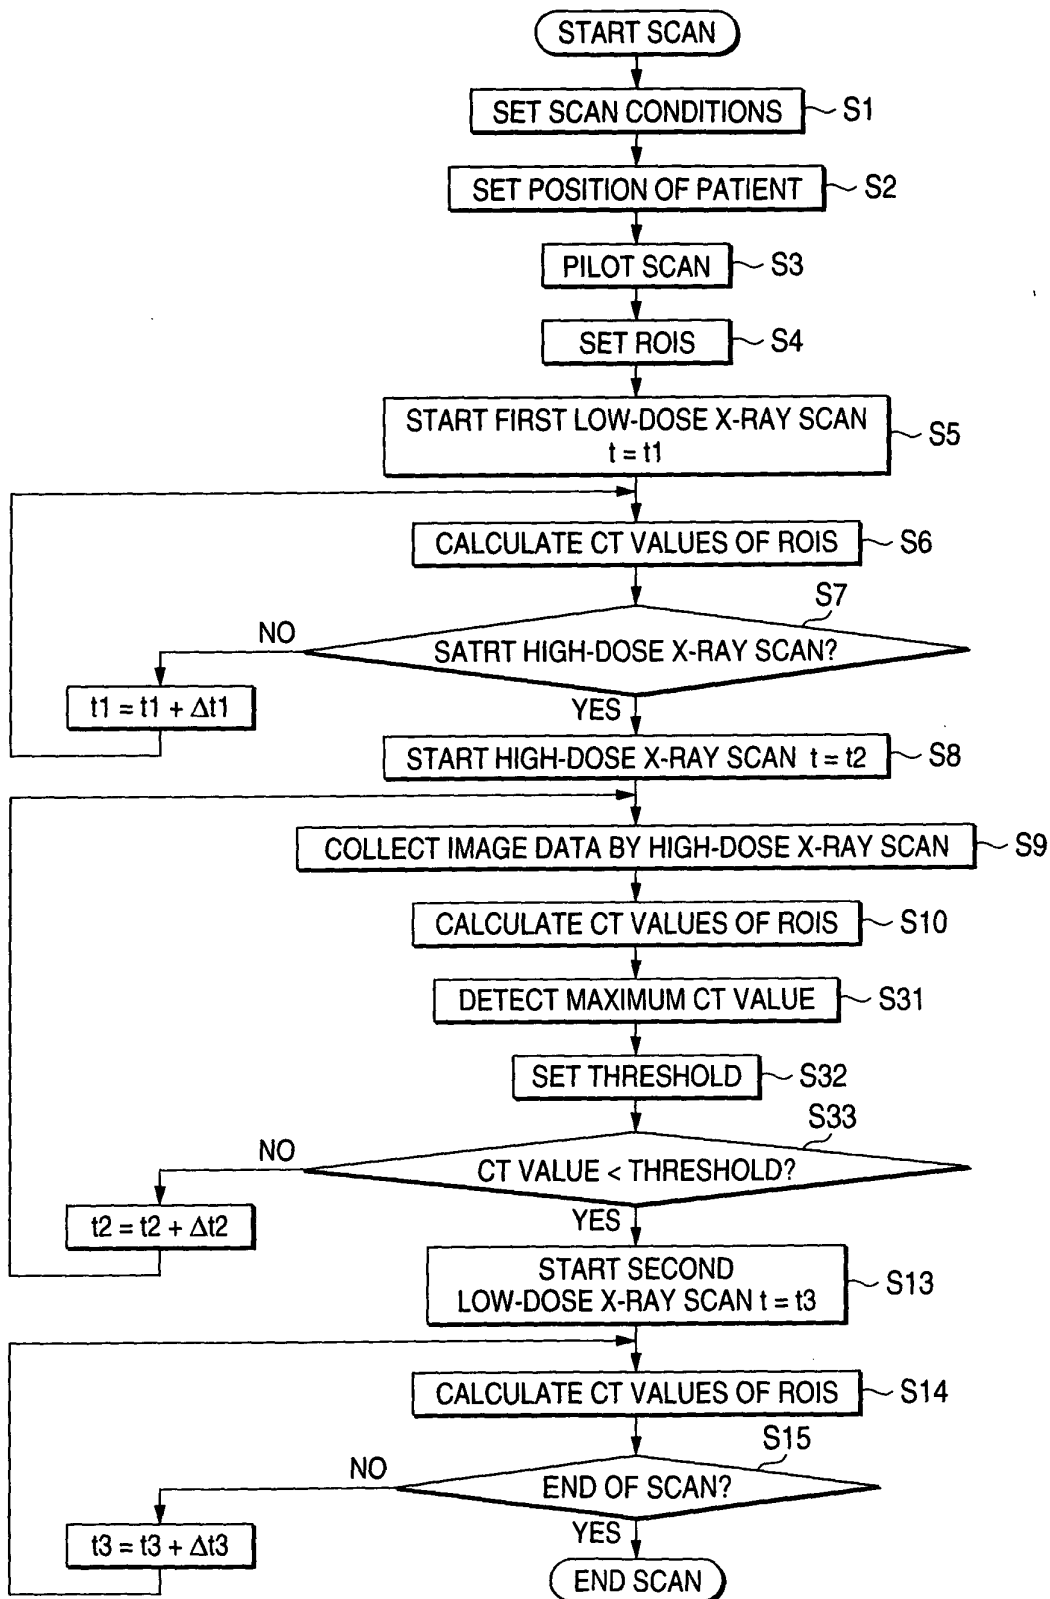


FIG. 14

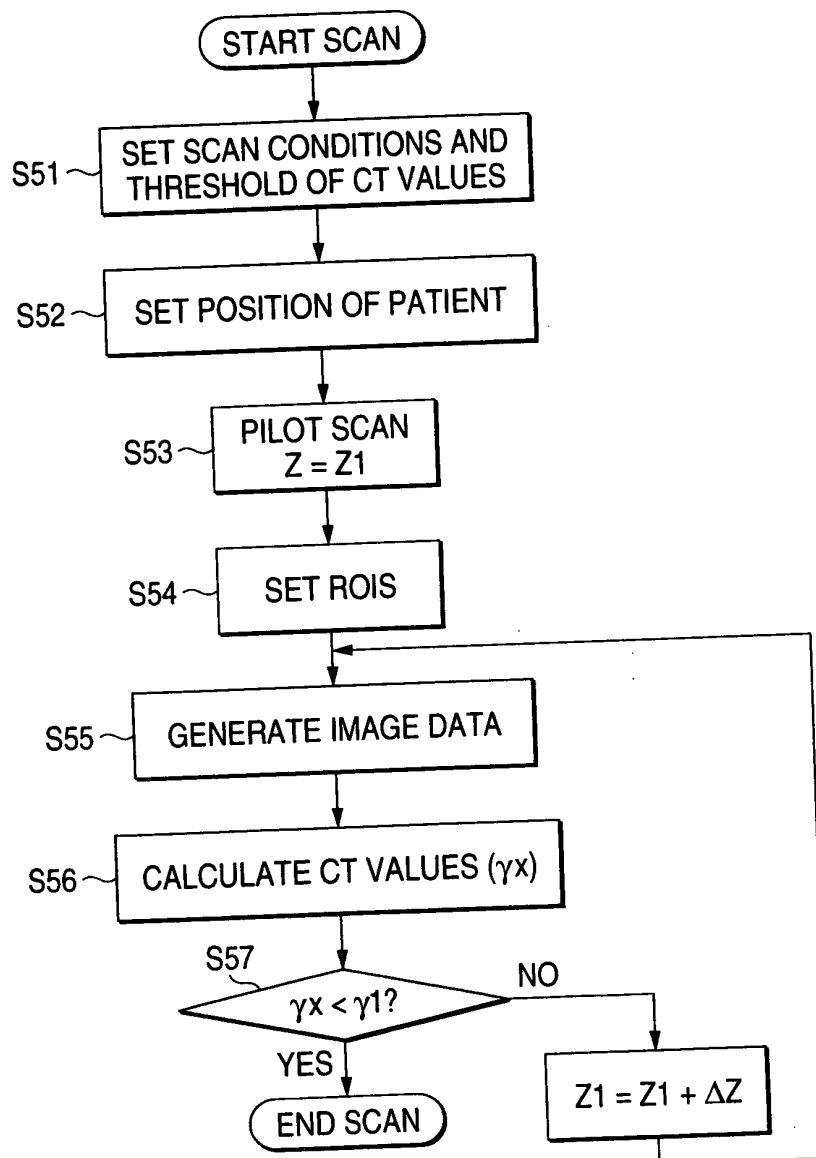


FIG. 15A



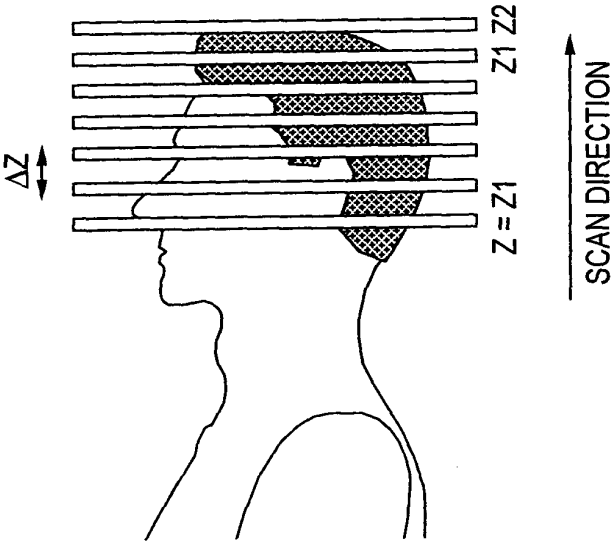


FIG. 15B

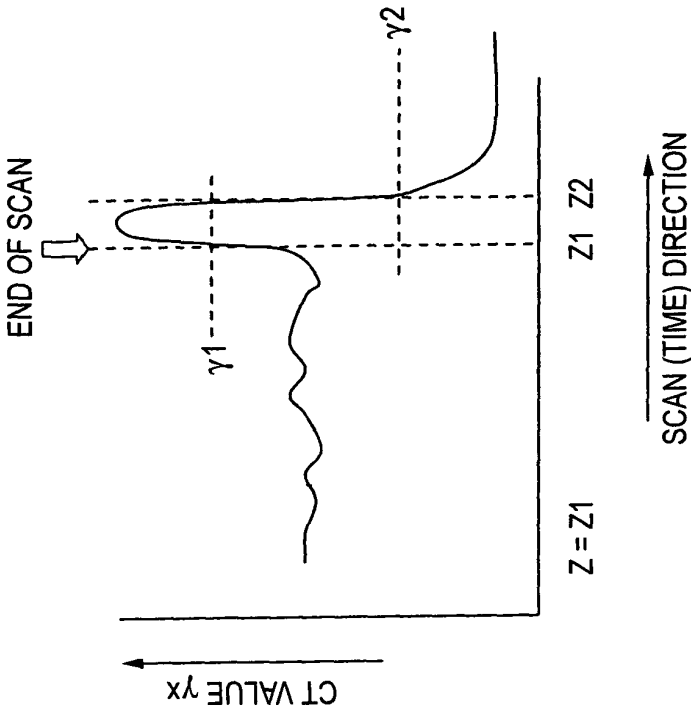

16/18

FIG. 16

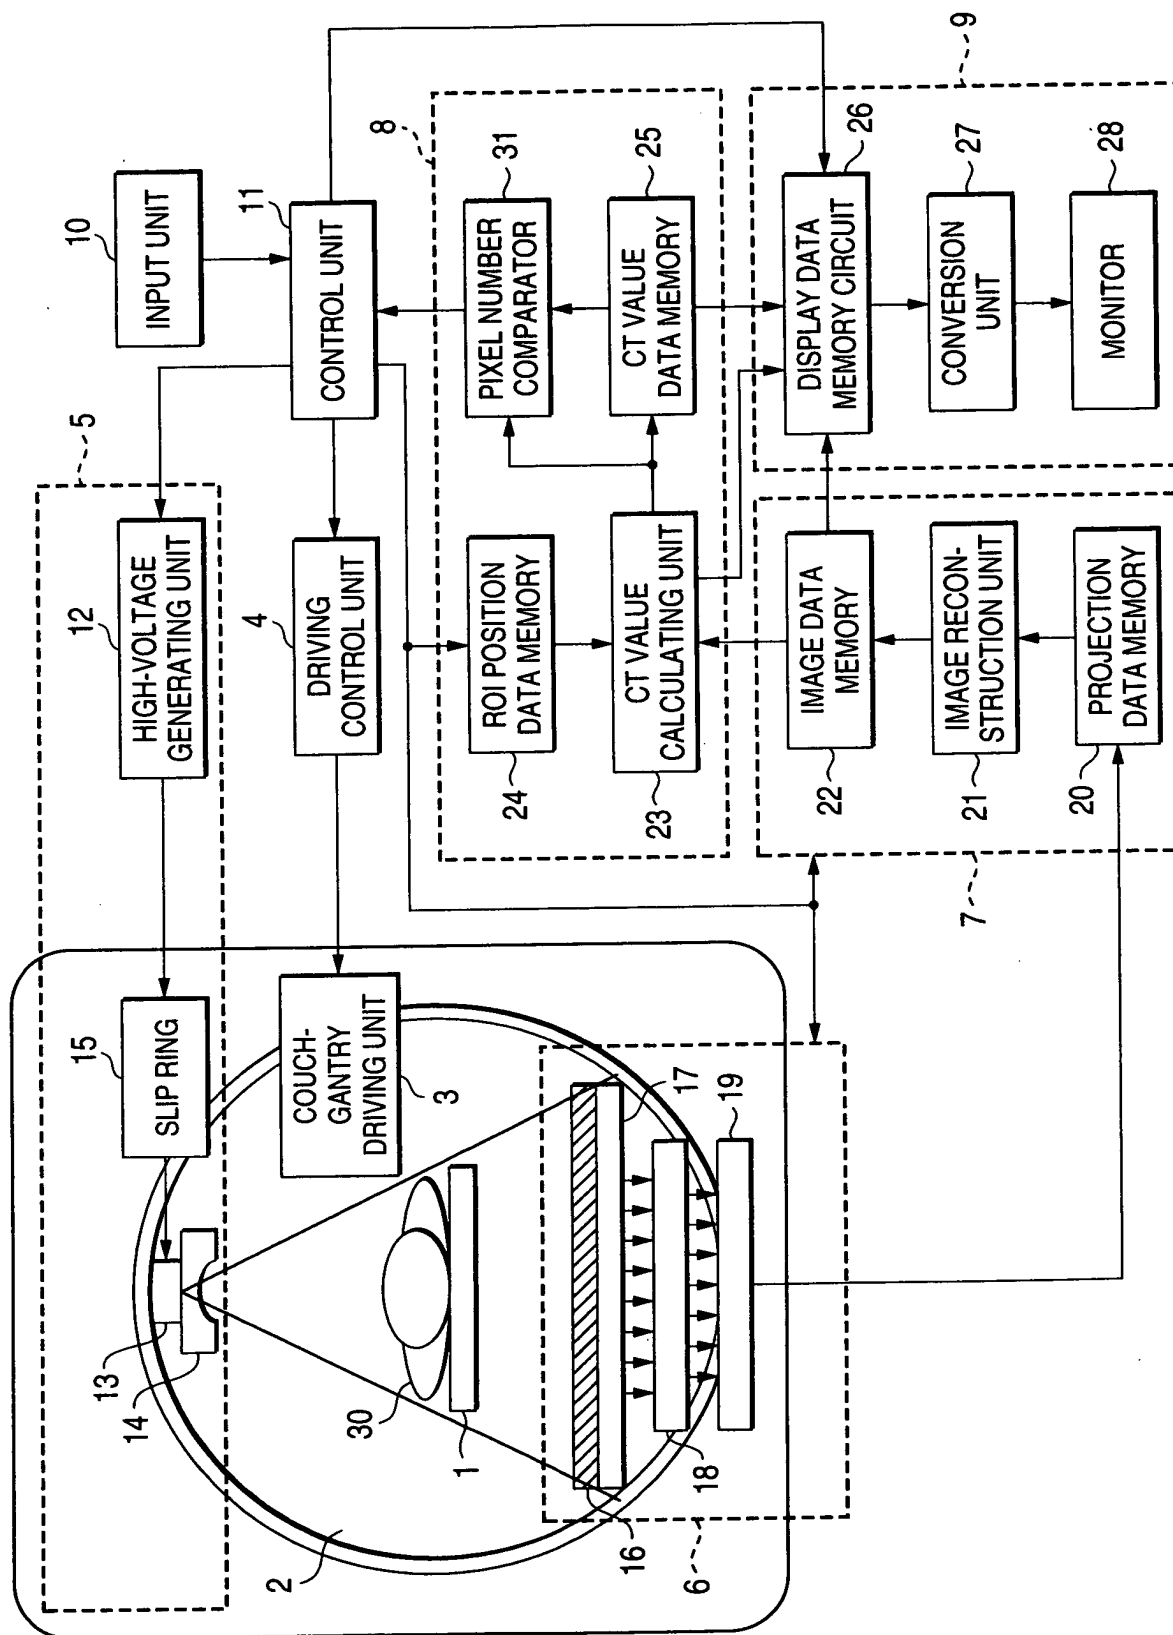

17/18

FIG. 17

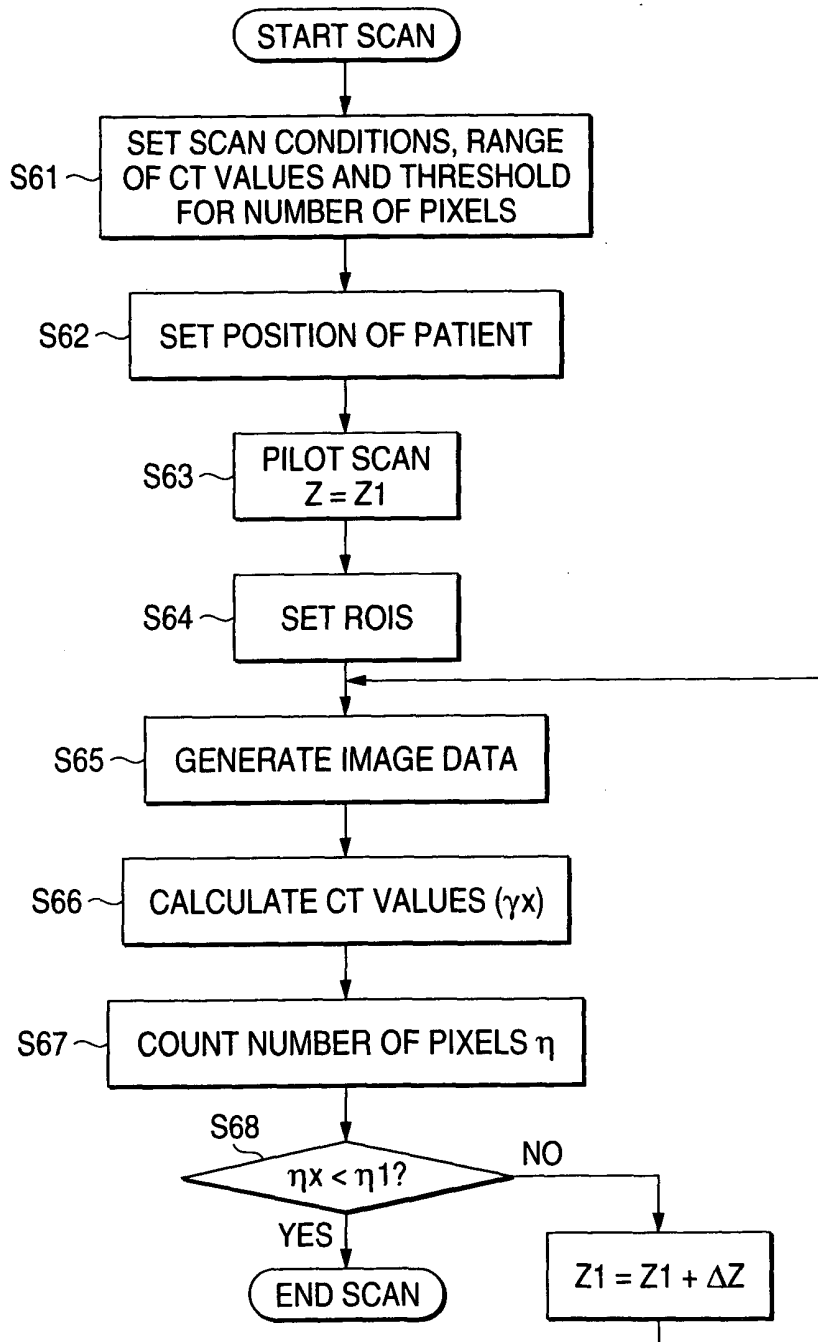


FIG. 18B

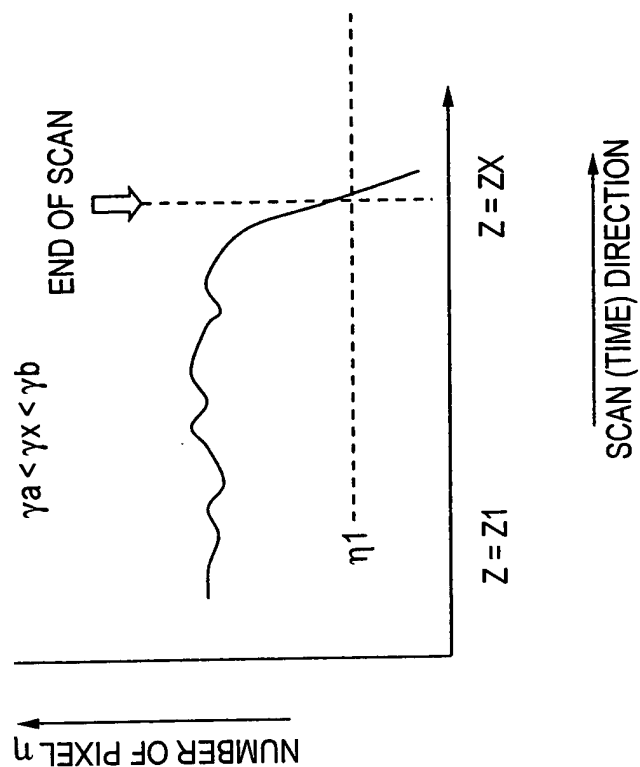


FIG. 18A

